Print on Plain White Paper (Part No. 122919)

MIDMARK®

Installation Instructions

9A205001/002 BASE RAIL ASSEMBLY

KIT COMPONENTS

Part Number	Description	Qty.
9A20500X	Base Rail Assembly	1 pair
003-0768-00	Installation / Operation Instructions	1

REQUIRED TOOLS

Punch (1/8” or smaller)
Needle Nose Pliers
3/8” Wrench
5/32” Hex Allen Wrench

INTRODUCTION

To provide a secure, stationary support for mounting certain accessories. Contains one pair, a patient’s right and left side, of Base Rail assemblies.

WARNING

Do not install on same side of table that has a 9A22700X Seat Rail. Remove any Seat Rails before installing the Base Rail. Failure to comply may result in personal injury or equipment damage.

INSTALLATION

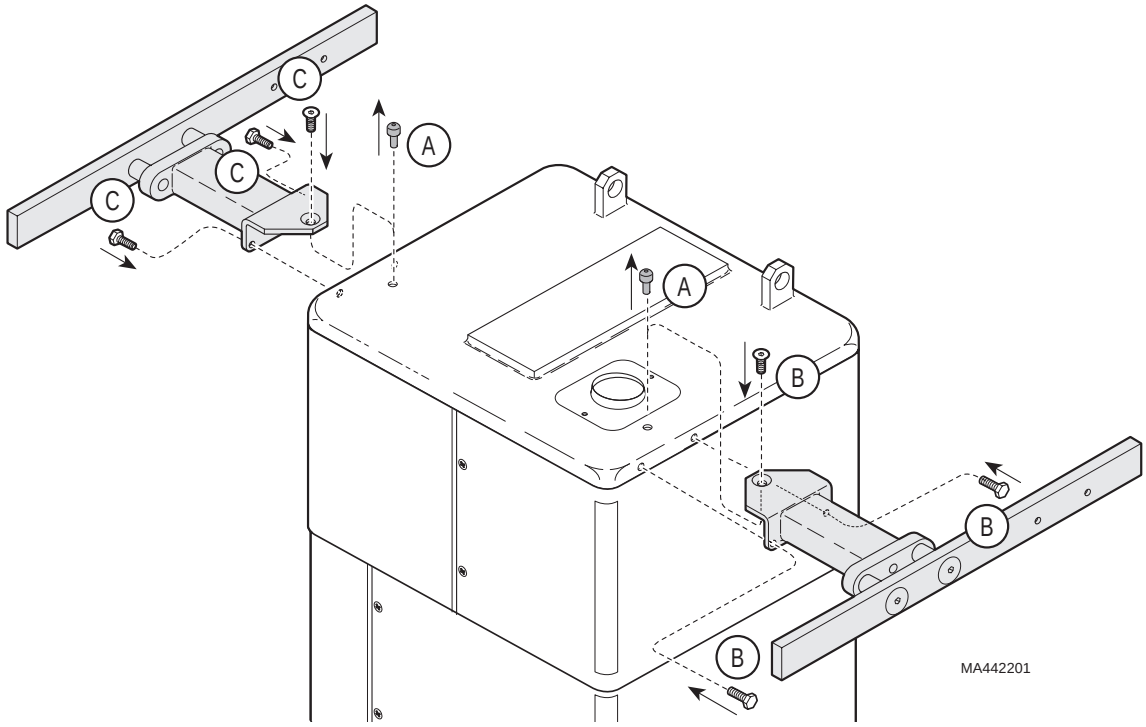

NOTE

For ease of installation, move TABLE, BACK, TILT and FOOT functions fully UP.

A. Using punch and pliers, remove black nylon rivets from mounting holes.

EQUIPMENT ALERT

The length of Base Rail that extends farther from base rail weldment must be pointed toward rear of table when mounting.

B. Place left-hand base rail in position and install mounting screws.

C. Install right-hand rail in similar manner.

MIDMARK®

Midmark Corporation, Versailles, Ohio 45380 U.S.A.
(937) 526-3662 FAX (937) 526-5542

003-0768-00 Rev. D (4/98)

© Midmark Corporation - 1998